





TENA SMARTCARE IDENTIFI™ SYSTEM INSTRUCTION MANUAL

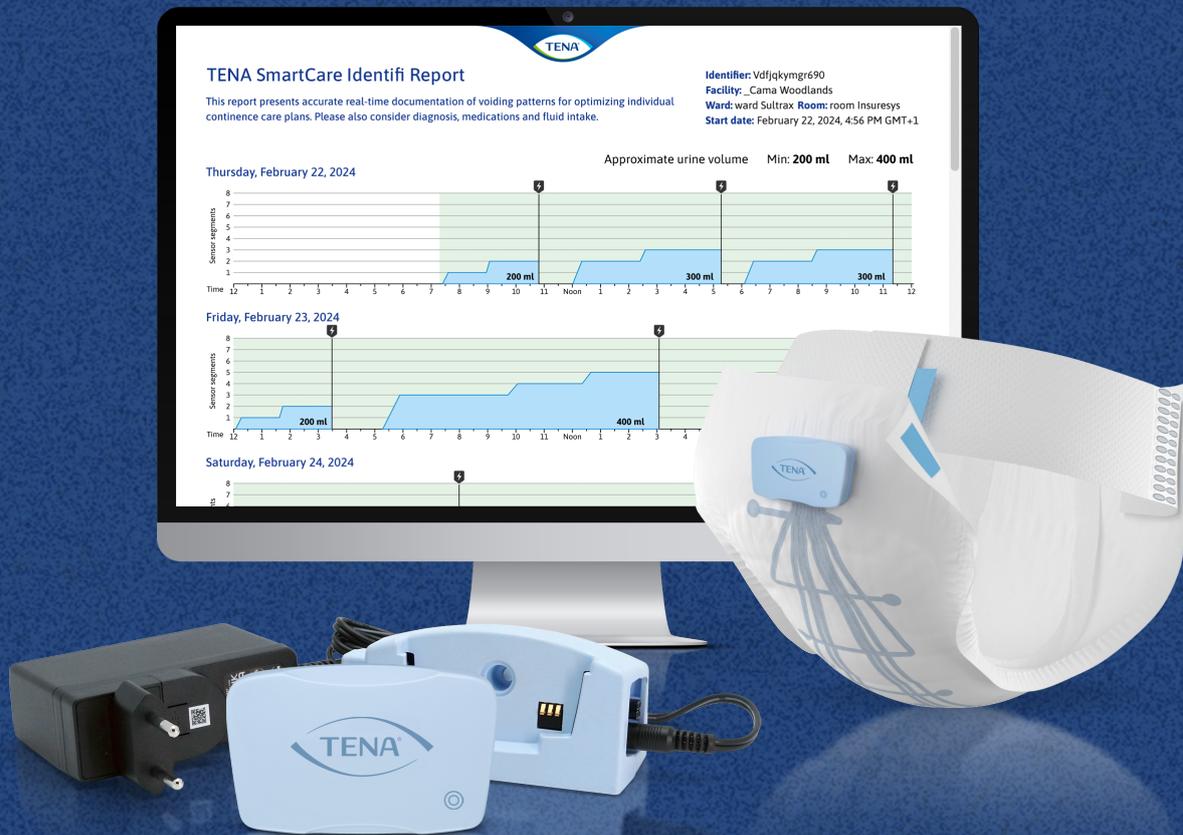


TENA SmartCare Identifi™

TENA SmartCare Identifi™ is a convenient and effective tracking system to support more accurate, individualized continence care plans.

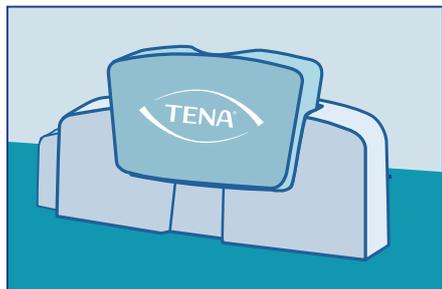


TENA SmartCare Identifi™ **Logger Kit** consists of a reusable logger and charger. The logger is used for recording and transmitting voiding data from TENA SmartCare Identifi™ Sensor Wear products.

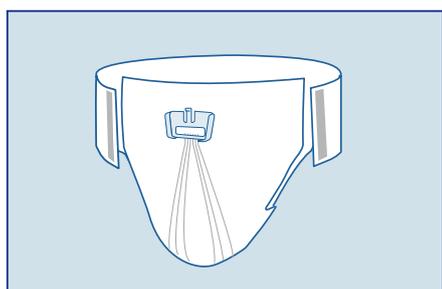

TENA SmartCare Identifi™ **Sensor Wear** is a disposable absorbent product with a logger connector and fine, thread-like sensors for collecting voiding information.



Data from the logger is automatically converted by the TENA SmartCare Identifi™ **Reporting System** into a report. The graphed report provides care staff with in-depth voiding patterns and other continence related information, to help support a more accurate, individualized continence assessment.



Light indications on the TENA SmartCare Identifi™ Logger

Light indication while attached to TENA SmartCare Identifi™ Sensor Wear:



Flashing green (flashes for 45 sec) = Correctly inserted



Steady orange = Low battery

Light indication while in charger unit:



Flashing orange = Charging



Steady green = Fully charged




Steady red = Out of order. Support needed, contact Essity Customer Service.

Before you start an assessment



Do not use TENA SmartCare Identifi™ **Logger** on individuals known to carry antibiotic resistant bacteria or contagious diseases.

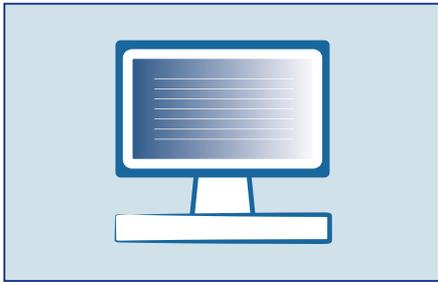

- 1 You need access to a computer with the internet browser open. Have your web portal user ID and password ready to access the TENA SmartCare Identifi™ Web Portal at this link: <https://tenaidentifi.essity.com>


Protect your personal password. It should not be shared with others. If you did not receive a user ID and temporary password, contact Essity Customer Service.



- 2 It is recommended to store the logger in the charger connected to a power source during the 72h assessment. Always store the logger safely away from exposure to sunlight and care takers when not in use. Make sure the logger has been charged for at least 2 hours and that it is fully charged. Check as follows:

Light indication while in charger unit:

-  Flashing orange = Charging
-  Steady green = Fully charged
-  Steady red = Out of order. Support needed, contact Essity Customer Service.

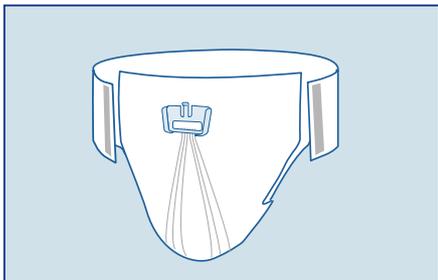

- 3 Make sure that you have an adequate supply of TENA SmartCare Identifi™ **Sensor Wear** to use for the 72 hr. period. Use Sensor Wear in place of other absorbent products for the 72 hr. assessment period. No other absorbent products such as pads, liners or briefs should be worn while **Sensor Wear** is in use.




- 4 Distribute TENA SmartCare Identifi™ toileting records, for manual documentation of the additional events to be captured on the 72 hr. report.



- 5 For successful results, do not operate the system without proper education and training from Essity/TENA staff or a trained designate.

Start an assessment

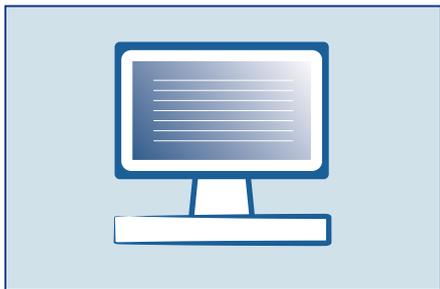


Log onto the web portal at <https://tenaidenti.essity.com> Register the assessment by connecting the TENA SmartCare Identifi™ Logger ID with the identifier of the person to be assessed. Refer to the TENA SmartCare Identifi™ Web Portal user manual for further instruction on starting the assessment in the web portal.



The TENA SmartCare Identifi™ Logger ID can be found on the label at the back of the logger. Make sure that the logger ID selected in the web portal matches with the logger ID selected for the assessment.

Handling of TENA SmartCare Identifi™ Sensor Wear and Logger during an assessment

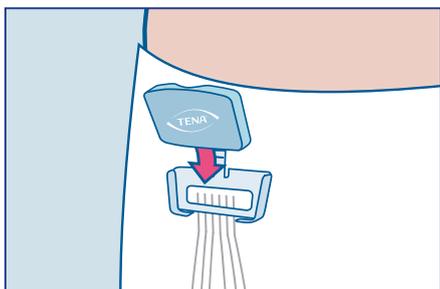

1 Attach TENA SmartCare Identifi™ Logger to TENA SmartCare Identifi™ Sensor Wear


Apply Sensor Wear as you would apply ordinary incontinence protection. Then insert the logger into the blue connector located at the front.

A flashing green light means the logger is correctly inserted. It stops flashing after 45 seconds and will remain idle until the next change. The logger is now ready to transmit data.



2 Record toileting events

Use a mobile device, tablet or diary-table for documentation of the additional events, e.g. toilet visits or leakage onto clothing/linen, to be included in the voiding report.

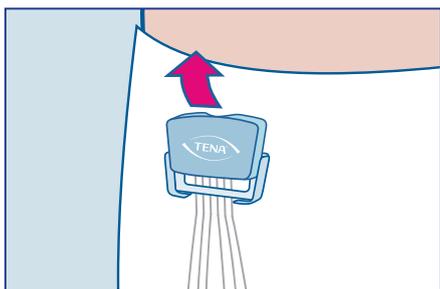

3 The TENA SmartCare Identifi™ Logger follows the resident

At next regular product change, apply protective gloves and slide the logger out of the connector, before taking off the Sensor Wear. The same logger is used during the whole assessment.



4 Discard used TENA SmartCare Identifi™ Sensor Wear. Be careful not to discard the logger!

Discard soiled Sensor Wear after the logger has been removed. Apply fresh Sensor Wear and insert the reusable logger into the connector. A flashing green light means the logger is correctly inserted.




5 If needed, recharge the TENA SmartCare Identifi™ Logger

Check for the solid orange 'low battery' light during Sensor Wear changes. If present, sanitise the logger according to the cleaning and disinfection protocol in this manual and then charge it for 30 minutes, before reinserting back into Sensor Wear connector.



6 Clean and disinfect TENA SmartCare Identifi™ Logger

When the assessment is finished, clean and disinfect the logger according to the cleaning and disinfection protocol in this manual. Once cleaned and charged, the logger is ready for a new assessment.

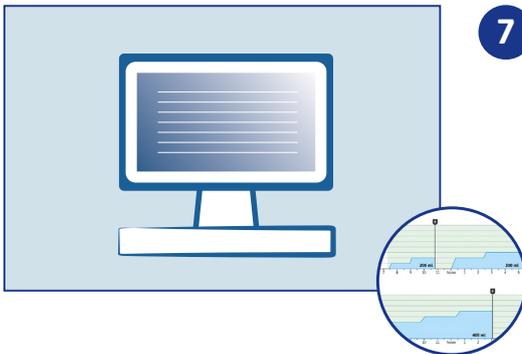

7 Complete voiding report in the TENA SmartCare Identifi™ Web Portal

After 72 hours, the residents go back to their regular products. If not already completed via a mobile device or tablet, register other continence-related data, such as toileting, leakage etc. in the web portal.

The TENA SmartCare Identifi™ Report is now ready to be analysed. Integrating TENA SmartCare Identifi™ into your assessment protocols provides care staff with more accurate information for improving continence care outcomes.

Cleaning instructions



Apply protective gloves before handling the logger and prior to cleaning and disinfection. Always clean and disinfect the logger before placing it back in the charger.



Do not use dishwasher or autoclave.



Do not use the TENA SmartCare Identifi™ Logger on individuals known to carry antibiotic resistant bacteria or contagious diseases. If the logger was mistakenly used on such individuals, follow your organization's infectious materials handling and infection control protocols.



The plastic surface of the TENA SmartCare Identifi™ Logger is compatible with the following non-corrosive disinfectants:

- hypochlorous solutions
- quaternary ammonium compound solutions

Do not use chlorine bleach (Sodium hypochlorite solution) on the logger device.



The charger should be cleaned off with a dry cloth to remove dust or similar. Liquid should be avoided.

Cleaning the logger



- 1 Clean every surface including crevices with water and detergent or pre-moistened cleaning wipe by rubbing the logger for at least 1 minute.



- 2 Dry the logger with a paper towel or disposable dry wipe. Proceed with disinfecting the logger as described below.



- 3 Disinfect the logger. Use a disinfectant suitable for low risk equipment to inactivate pathogen microorganisms. Example disinfectant products are:
 - 70% alcohol
 - Virkon® containing the active ingredient hypochlorous solutionRub every surfaces including crevices and make sure surfaces and crevices are completely saturated with the disinfectant. Follow the manufacturer's recommended instructions for use of the disinfectant.

Virkon is a registered trademark of E. I. du Pont de Nemours and Company or its affiliates.



- 4 Allow the logger to air-dry completely. The logger is now ready to place back in the charger.

Cautions:

Warning! Only use the power cord and charging unit provided in the TENA SmartCare Identifi™ Logger Kit.

Warning! Only connect a maximum of 3 charging units in a series to a single power supply.

Warning! If any of the contents of the TENA SmartCare Identifi™ Logger kit appear to be damaged or broken, contact TENA Customer Service.

Warning! Before extended storage of the logger, always charge the logger first. A drained battery severely decreases the battery functionality.

Warning! Do not use the TENA SmartCare Identifi™ Logger on individuals known to carry antibiotic resistant bacteria or contagious diseases.

Important:

Save this instruction manual for future reference.

Read all instructions carefully and completely before initiating an assessment. If in doubt, contact Essity for support.

Avoid placing the equipment in direct sunlight as it will discolor the plastic casings.

Always clean and disinfect the TENA SmartCare Identifi™ Logger unit in accordance with this manual.

No modification of this equipment is allowed.

IP65 rating: 6 Dust-tight, 5 Protected against water jets.

TENA SmartCare Identifi™ Logger Kit must be **returned** to Essity after the end of its service life.



For the latest version of this document please visit <https://tenaidentifi.essity.com>

Computer not included. Reporting system can be accessed from any available computer with internet. Logger and Sensor wear shown are not the actual size. TENA SmartCare Identifi™ Sensor Wear sold separately.

TENA is a registered trademark of Essity Hygiene and Health AB.



Essity Hygiene and Health AB
SE-405 03 Göteborg, Sweden
Visiting address:
Mölnåls Bro 2, Mölnåls
www.essity.com



essity

TENA
an Essity brand

